

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00746 Calib. Date: 12/13/2018 Calib. No.: 00029
Certification File No.: 00747 Cert. Date: 12/13/2018 Cert. No.: 00023
Linearity File No.: 00748 Lin. Date: 12/13/2018 Lin. No.: 00023
Solution File No.: 00768 Soln. Date: 04/15/2019 Soln. No.: 00158
Sequential File No.: 00768 File Date: 04/15/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0216
Control Solution %: 0.100% Expires: 06/28/2019
Solution Control Lot: 17200 Bottle No.: 1436

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:19D		
Control 1 EC	0.098%	10:19D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:20D		
Control 2 EC	0.098%	10:21D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	10:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:22D		
Control 3 EC	0.098%	10:23D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	10:23D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:24D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: VALDES

First Name: HEATHER

MI: -

Signature: _____

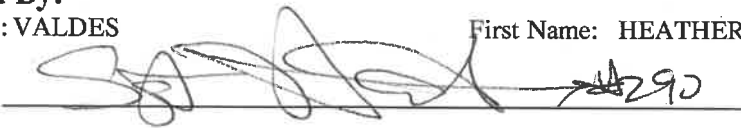

Badge No.: 290

Date: 04/15/2019