

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0056
Location:	LONG BRANCH POLICE DEPT		
Calibration File No.:	00665	Calib. Date:	04/04/2017
Certification File No.:	00666	Cert. Date:	04/04/2017
Linearity File No.:	00667	Lin. Date:	04/04/2017
Solution File No.:	00679	Soln. Date:	06/18/2017
Sequential File No.:	00679	File Date:	06/18/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXN S3-0217
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	1332

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:56D		
Control 1 EC	0.100%	00:57D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	00:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:58D		
Control 2 EC	0.099%	00:59D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	00:59D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:59D		
Control 3 EC	0.098%	01:00D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: VALDES

First Name: HEATHER

MI: -

Signature: _____

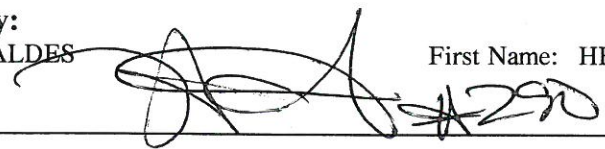

Badge No.: 290

Date: 06/18/2017