


# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C  
Serial No.: ARXA-0056  
Location: LONG BRANCH POLICE DEPT  
Calibration File No.: 00713 Calib. Date: 07/17/2018 Calib. No.: 00028  
Certification File No.: 00683 Cert. Date: 09/14/2017 Cert. No.: 00021  
Linearity File No.: 00684 Lin. Date: 09/14/2017 Lin. No.: 00021  
Solution File No.: 00710 Soln. Date: 01/26/2018 Soln. No.: 00147  
Sequential File No.: 00713 File Date: 07/17/2018


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0217  
Control Solution %: 0.100% Expires: 08/07/2019  
Solution Control Lot: 17230 Bottle No.: 1022

## Coordinator

Last Name: PAVLOSKY First Name: ALLISON MI: M.  
Signature:  Badge No.: 7330  
Date: 07/17/2018

\*Black Key Temperature Probe Serial.....# DDXK P2 - 398 A

\*Digital NIST Temperature Measuring System Serial.....# 170428364 A

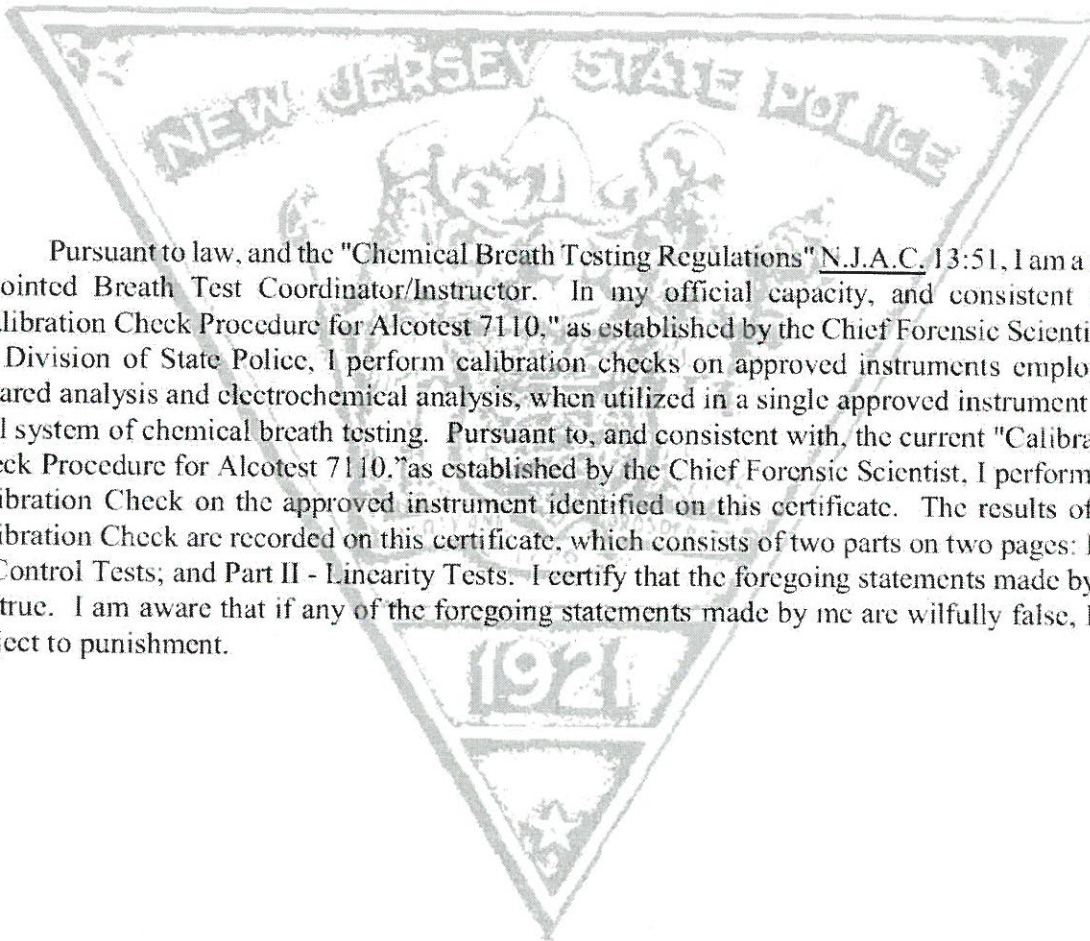

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.