

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00682
Calib. Date: 09/14/2017
Calib. No.: 00027
Certification File No.: 00666
Cert. Date: 04/04/2017
Cert. No.: 00020
Linearity File No.: 00667
Lin. Date: 04/04/2017
Lin. No.: 00020
Solution File No.: 00679
Soln. Date: 06/18/2017
Soln. No.: 00139
Sequential File No.: 00682
File Date: 09/14/2017

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDXN S3-0217
Control Solution %: 0.100%
Expires: 09/07/2018
Solution Control Lot: 16220
Bottle No.: 0378

Coordinator

Last Name: ALCOTT
First Name: KEVIN
MI: W.
Signature: Tpr. I K W. #6704
Badge No.: 6704
Date: 09/14/2017

*Black Key Temperature Probe Serial.....# ΔΔHH92-065 (KA)
*Digital NIST Temperature Measuring System Serial.....# 170 428 368 (KA)

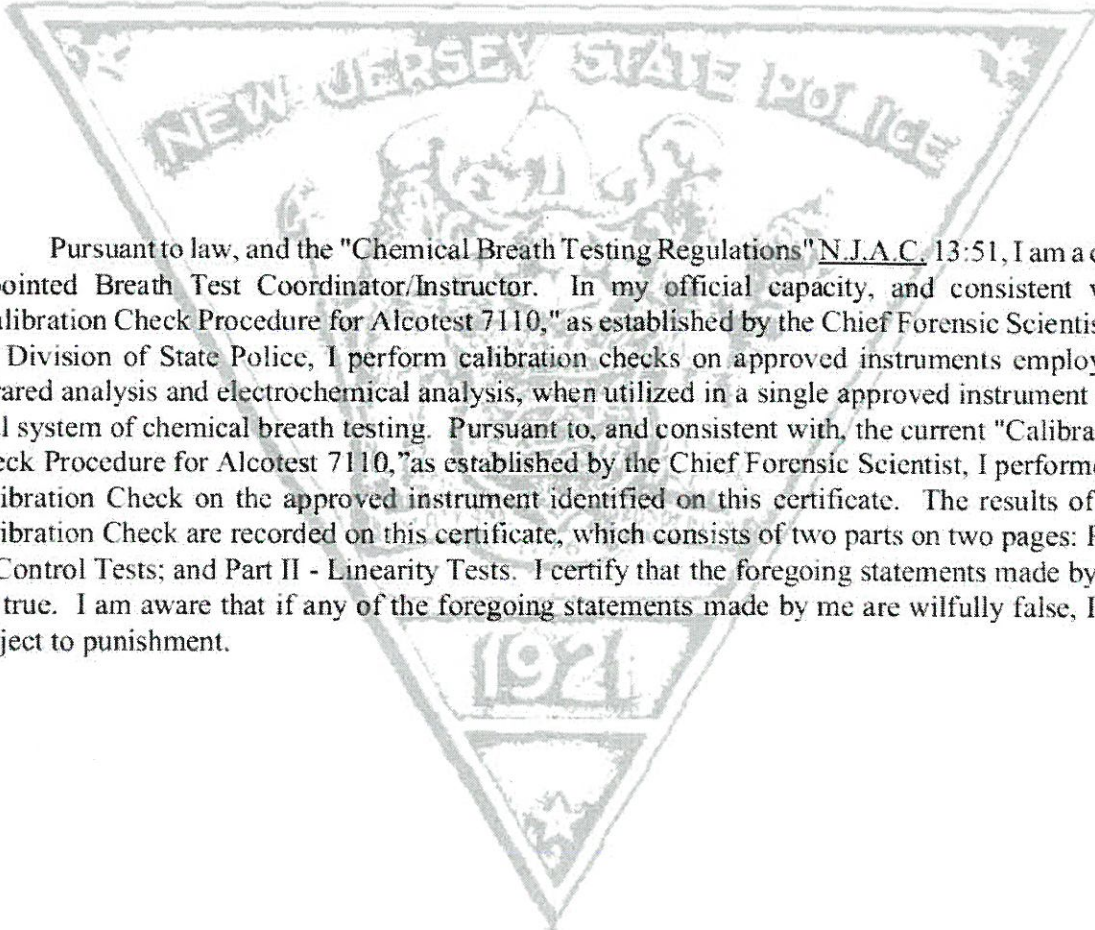

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.