

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
Location: LONG BRANCH POLICE DEPT
Serial No.: ARXA-0056
Calibration File No.: 00746
Certification File No.: 00714
Linearity File No.: 00715
Solution File No.: 00745
Sequential File No.: 00746
Calib. Date: 12/13/2018
Cert. Date: 07/17/2018
Lin. Date: 07/17/2018
Soln. Date: 12/09/2018
File Date: 12/13/2018
Calib. No.: 00029
Cert. No.: 00022
Lin. No.: 00022
Soln. No.: 00153


Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 17230
Model No.: CU-34
Serial No.: DDXN S3-0216
Expires: 08/07/2019
Bottle No.: 0846

Coordinator

Last Name: NAPOLITANO
First Name: DAVID
MI: M.
Signature: *David M. Napolitano* 7237
Badge No.: 7237
Date: 12/13/2018

*Black Key Temperature Probe Serial.....# DDXK P2-396 (DN)

*Digital NIST Temperature Measuring System Serial.....# 170 297 886 (DN)

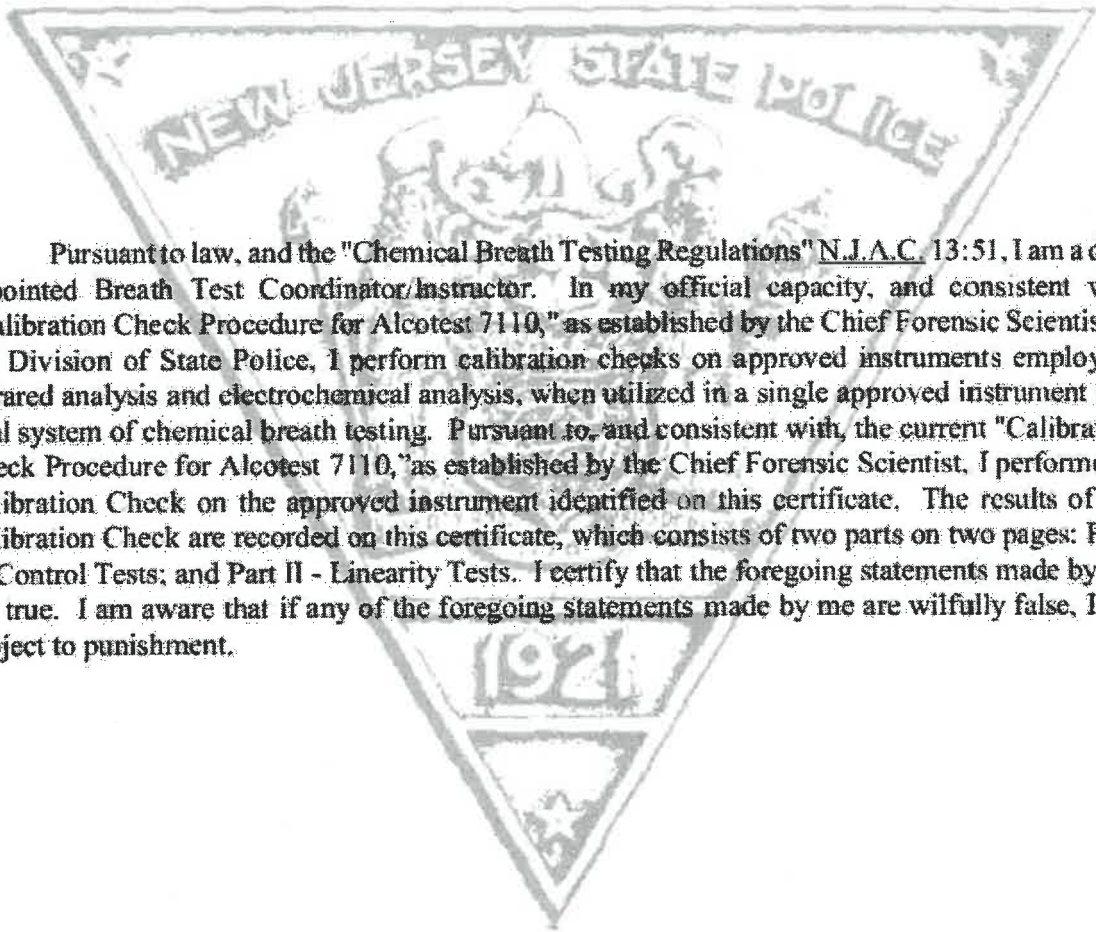

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0056
Location: LONG BRANCH POLICE DEPT
Calibration File No.: 00746 Calib. Date: 12/13/2018 Calib. No.: 00029
Certification File No.: 00747 Cert. Date: 12/13/2018 Cert. No.: 00023
Linearity File No.: 00715 Lin. Date: 07/17/2018 Lin. No.: 00022
Solution File No.: 00745 Soln. Date: 12/09/2018 Soln. No.: 00153
Sequential File No.: 00747 File Date: 12/13/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0216
Control Solution %: 0.100% Expires: 08/07/2019
Solution Control Lot: 17230 Bottle No.: 0846

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:13S		
Control 1 EC	0.099%	12:14S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:14S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:15S		
Control 2 EC	0.099%	12:15S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	12:15S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:16S		
Control 3 EC	0.098%	12:17S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	12:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:18S		

All tests within acceptable tolerance.

Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: 

Badge No.: 7237

Date: 12/13/2018

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0056
Location:	LONG BRANCH POLICE DEPT	
Calibration File No.:	00746	Calib. Date: 12/13/2018
Certification File No.:	00747	Cert. No.: 00023
Linearity File No.:	00748	Lin. Date: 12/13/2018
Solution File No.:	00745	Lin. No.: 00023
Sequential File No.:	00748	Soln. No.: 00153
		File Date: 12/13/2018
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.040%	Serial No.: DDWE S3-0206
Solution Control Lot:	17240	Expires: 08/10/2019
		Bottle No.: 1155
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.080%	Serial No.: DDWF S3-0218
Solution Control Lot:	17250	Expires: 08/15/2019
		Bottle No.: 0961
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.160%	Serial No.: DDWJ S3-0334
Solution Control Lot:	17260	Expires: 08/21/2019
		Bottle No.: 0658

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:28S		
Control 1 EC	0.040%	12:28S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.040%	12:28S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30S		
Control 2 EC	0.040%	12:31S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.039%	12:31S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32S		
Control 3 EC	0.081%	12:33S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	12:33S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:35S		
Control 4 EC	0.081%	12:36S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.078%	12:36S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:38S		
Control 5 EC	0.161%	12:38S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.157%	12:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:40S		
Control 6 EC	0.159%	12:41S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.156%	12:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:43S		

All tests within acceptable tolerance.

Coordinator

Last Name: NAPOLITANO

First Name: DAVID

MI: M.

Signature: _____

David Napolitano 7237

Badge No.: 7237

Date: 12/13/2018